


Supplementary Figure 14. Subgroup analysis of the rate of atrial fibrillation detection with implantable cardiac monitors, stratified by the elapsed time between ischemic stroke/transient ischemic attack onset and implantation of cardiac monitor (≤ 1 and > 1 month), in all included studies. CI, confidence interval; EV/Trt, events/treated.

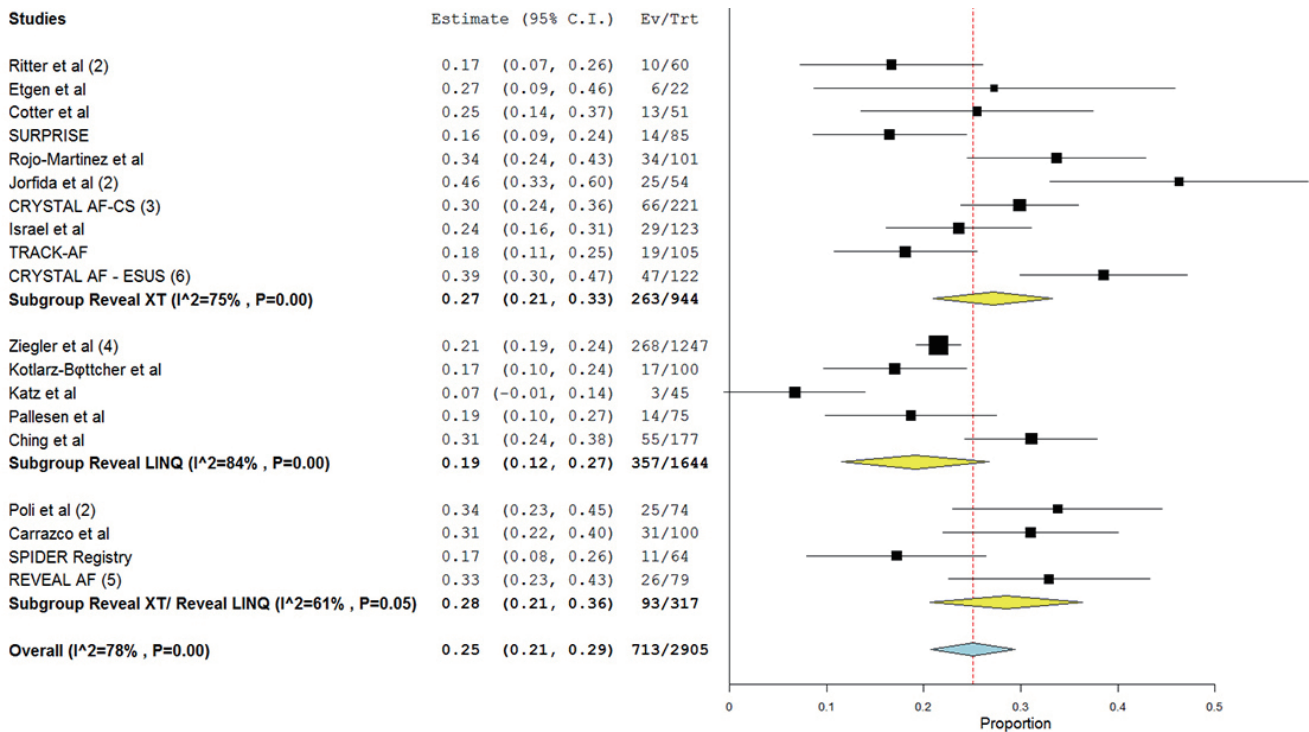

Supplementary Figure 15. Subgroup analysis of the rate of atrial fibrillation detection with implantable cardiac monitors, stratified by the type of device used, in all included studies. CI, confidence interval; EV/Trt, events/treated.