


Supplementary Figure 20. Subgroup analysis of the rate of atrial fibrillation detection with implantable cardiac monitors, stratified by the type of device used, in all included studies. CI, confidence interval; EV/Trt, events/treated.

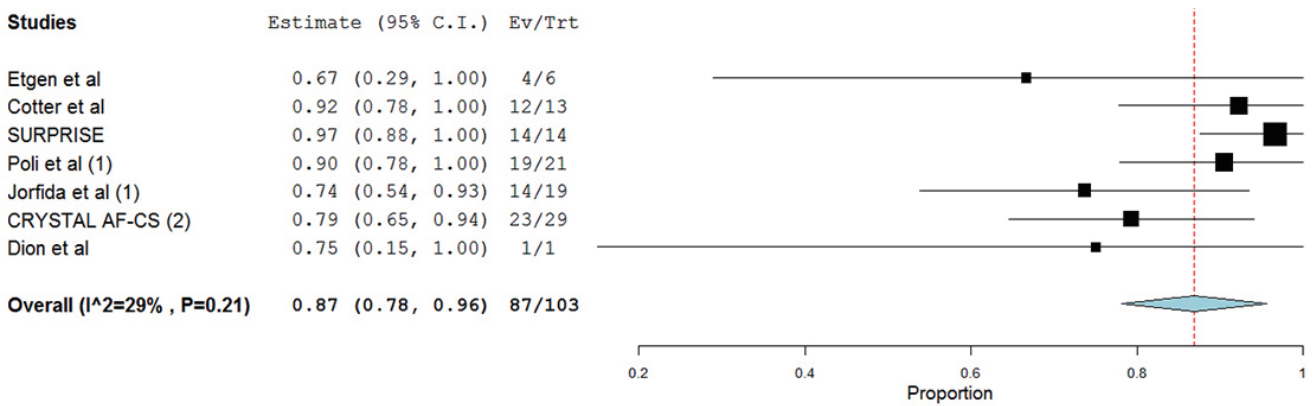

Supplementary Figure 21. Pooled analysis of the proportion patients with episodes of asymptomatic atrial fibrillation, among patients with episodes of atrial fibrillation (both asymptomatic and symptomatic) detected with implantable cardiac monitoring. CI, confidence interval; EV/Trt, events/treated.